


-15kV TOF: -9181 v  
 -3.6kV MCP: -2971 v  
 -2.4kV MCP: -1774 v  
 Input Cur: 300 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Thu Dec 21 06:20:50 2006

## TIDE Direct Events

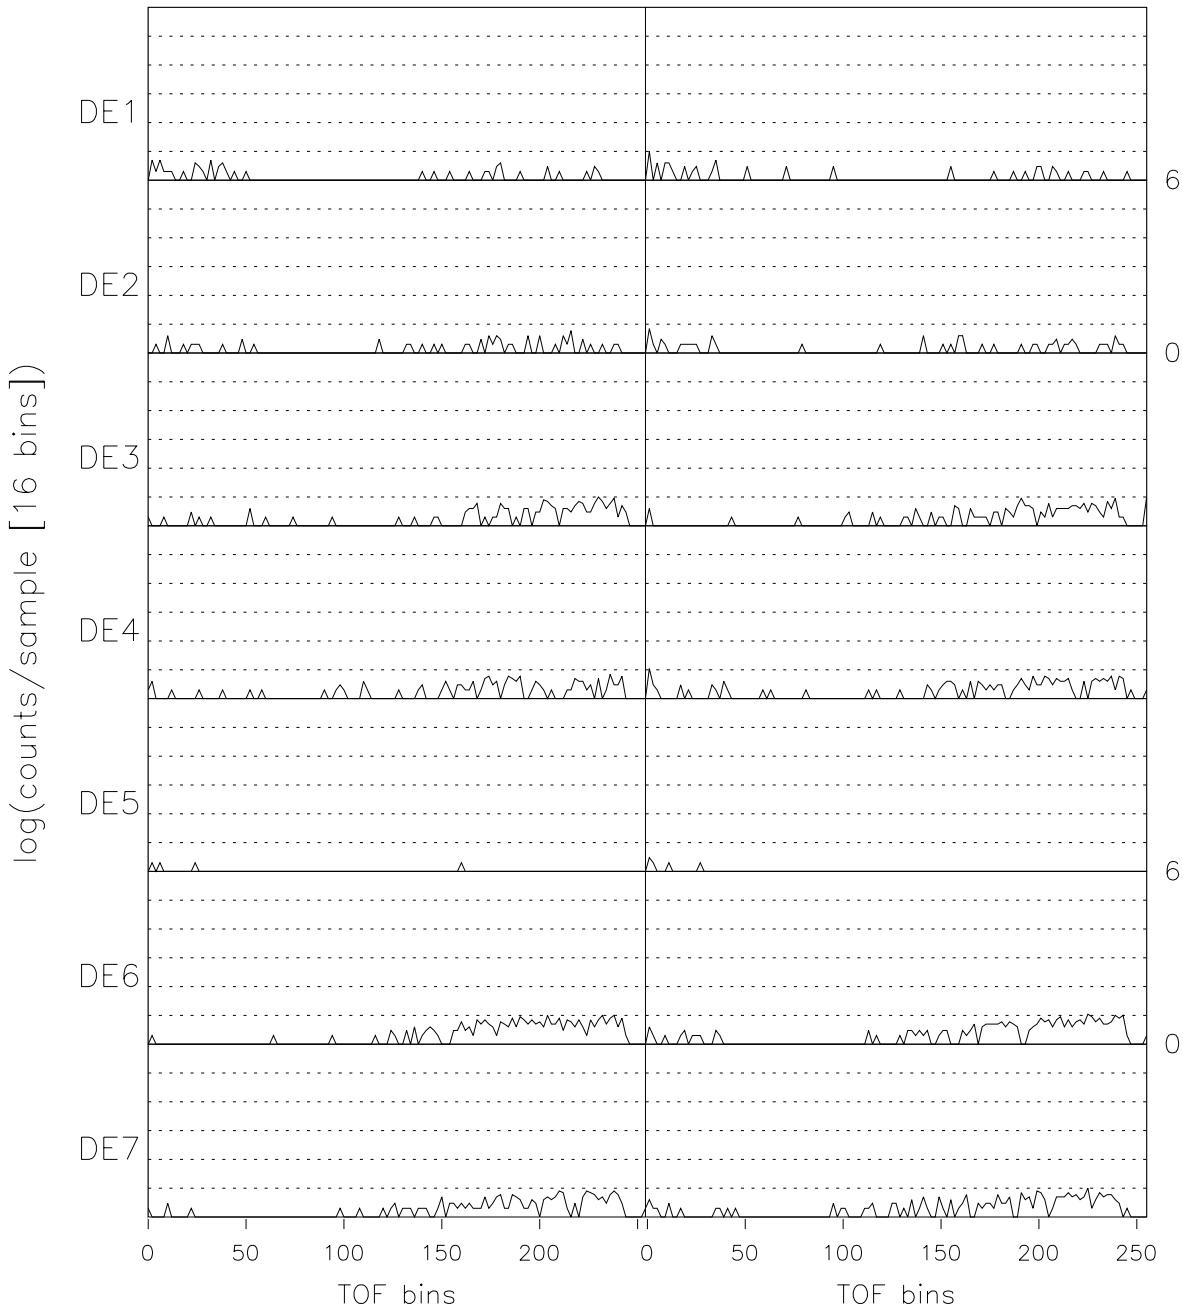

reported: 12-21-06 06:13:49 UT

reported: 12-21-06 06:17:01 UT

file: /export/data/tide/nrt/nrt0612210605.lz

-15kV TOF: -9181 v

-3.6kV MCP: -2986 v

-2.4kV MCP: -1774 v

Input Cur: 310 ma

RPA max: 237 v

Mirror max: 238 v